



Filter media test rig in accordance to **DIN EN 1822-3** and **ISO 29463-3** with U-SMPS for determination of MPPS range

Description

MFP filter test rigs from Palas® have already proved themselves many times over all around the world in practical applications in development and quality control.

MFP Nano plus has been specially designed for the clear determination of the separation efficiency of HEPA and ULPA filter media in accordance with DIN EN 1822-3 and ISO 29463-3.

the form of the **U-SMPS**, a modern and powerful nano particle measuring device with a measurement range from 5 nm to 1 µm is used for particle size and quantity analysis.


the aid of the universal aerosol generator UGF 2000, defined aerosol distributions matched to the MMPS range can be produced with DEHS or salt (NaCl / KCl).

Thanks to the movable dilution cascades, the test rig can be changed over from salt aerosols to DEHS aerosols within a very short space of time, with no need for cleaning.

largely automated setup of the test sequence together with the clearly defined individual components and the individually adjustable sequence programs of the filter test software FTControl combine to deliver the high reliability of our measurement results.

MFP filter test rig is a modular filter testing system for flat filter media and small mini-filters. loss curves, fraction separation efficiency or burden can be determined within a very short period of time – both reliably and cost-effectively. **Our quality in detail**

MFP Nano plus

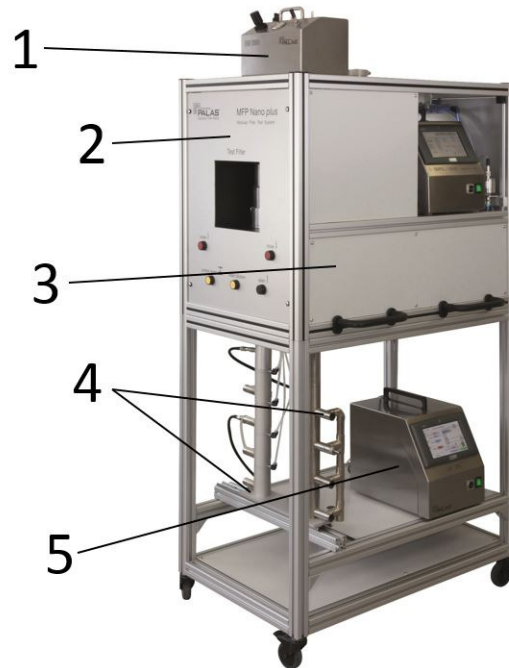

1. **Variable aerosol generation** with the UGF 2000 for KCl / NaCl or DEHS. Integrated silica gel drying length. The volume flow for the aerosol generation is individually regulated via mass flow controllers. 2. **Aerosol neutralization: Krypton source Kr 85 - 370 or Soft x-ray Charger XRC 370**

Corona discharge (optional): Adjustable ion stream for different mass flows. Adjustable mixed air for inflow speeds from 1.5 to 40 cm/s. Monitoring and control are implemented via mass flow controllers. 3. **Mobile pneumatic filter holder** for fast removal and loading of the test rig. 4. **Movable dilution cascades:** dilution cascades enable defined dilution of the applied test aerosol by the factors 10, 100, 1,000 and 10,000. As they are movable, the test rig can be changed over in a very short time from salt aerosols to DEHS aerosol. Lengthy or complex cleaning of the systems is not required. 5. **U-SMPS for nano particle measurement** Palas® filter test software FTControl controls the U-SMPS and evaluates the data. **Adjustment of the aerosol distribution to the MPPS range** Through suitable adjustment of the solution concentration, the generated particle size distribution is matched to the relevant MPPS range in the MFP Nano plus.

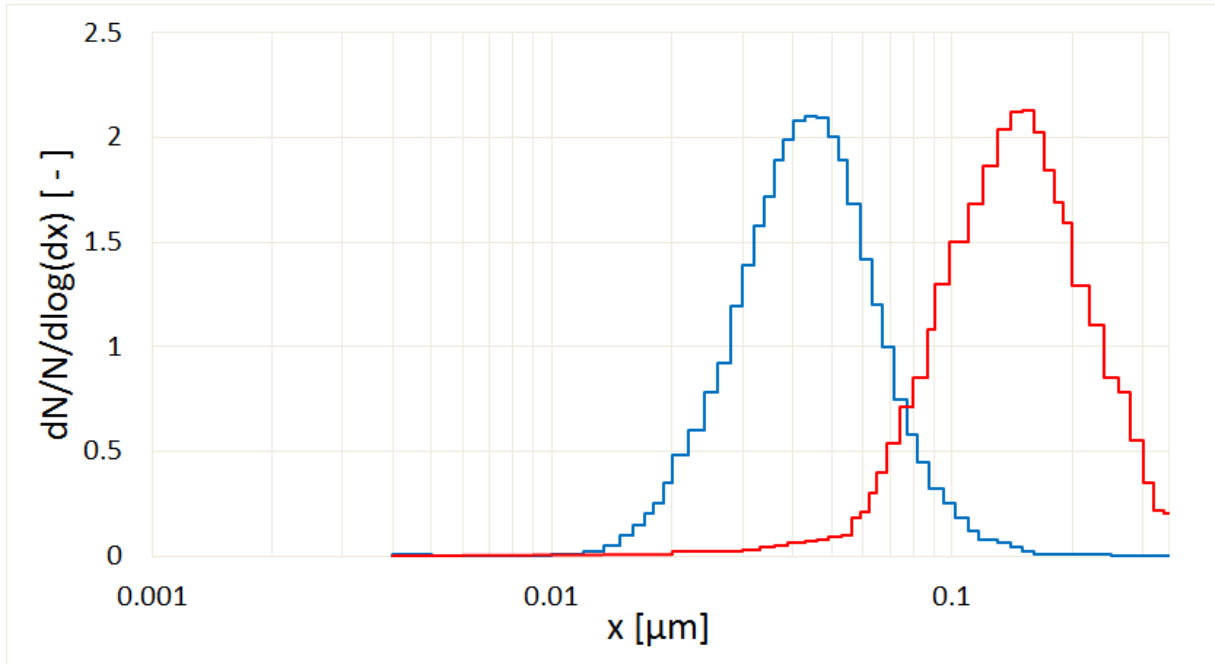


Fig. 1: Adjustment of the particle sizes for the required MPPS range with DEHS

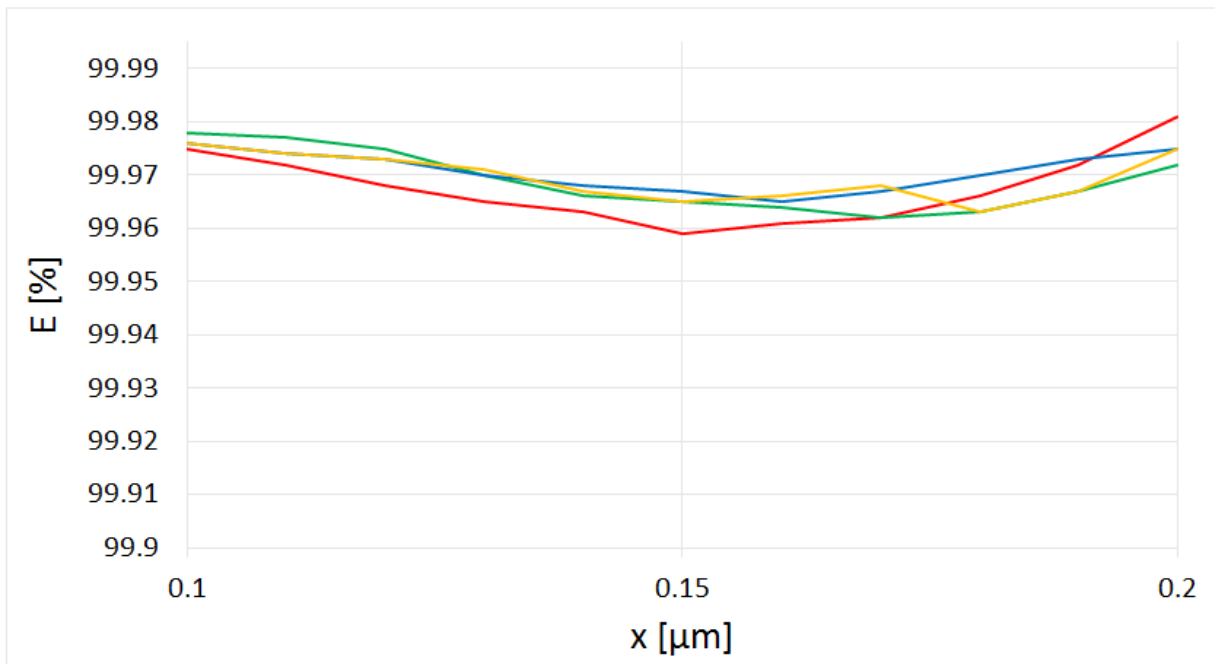


Fig. 2: Comparison of fraction separation efficiencies in the MPPS range at 140 nm

- Clear demonstration of the separation efficiency of the filter medium throughout the entire measurement range
- Clear determination of the MPPS range

- Highest measurement reproducibility and repeatability highlight even fine differences in the separation efficiency
- Short measurement times of around 6 minutes per separation efficiency measurement thanks to optimized application
- Simple comparison of separation efficiency curves, calculation of mean values also possible

Automation: MFP Nano *plus* has integrated mass flow controllers that it uses to control the volume flow; these can be automatically monitored and controlled via the FTControl filter test software. Data such as the volume flow and differential pressure at the filter are also recorded automatically during the filter test. The raw gas measurement is performed without the filter medium with a dilution factor matched to the separation efficiency (10, 100, 1,000 or 10,000). The clean gas measurement is then performed without dilution and with the filter medium inserted. The change in dilution factor is performed automatically.

Verification of the dilution factor: dilution systems integrated in the MFP Nano *plus* work in the same way as the tried and tested VKL series with the ejector principle. The advantages of this dilution cascade are the clear transfer behavior, low level of contamination and the simple cleaning.

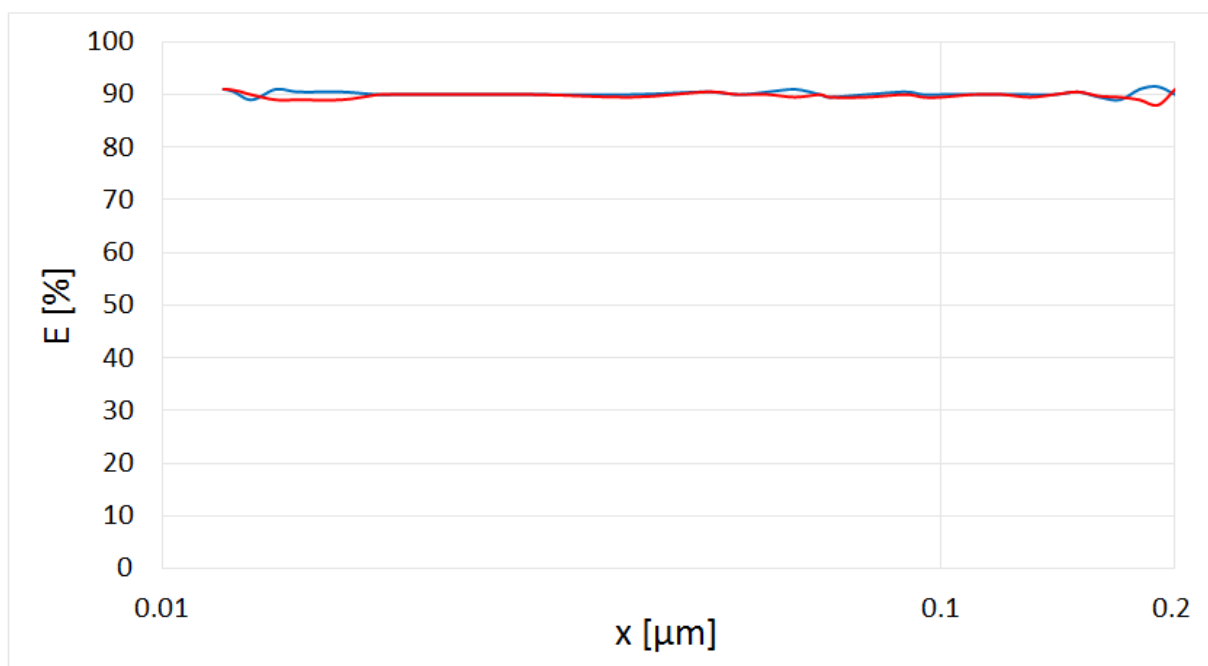


Fig. 3: Verification of the dilution factor via raw/clean gas comparison with a factor of 10 and NaCl particles

- With the MFP Nano *plus*, measurements of the fraction separation efficiency can be performed both in the MPPS range and across the entire measurement range. In addition, the relevant pressure loss of the medium is clearly determined at the relevant inflow speed.

Benefits

- Particle size measurements from 10 nm
- Internationally comparable measurement results in accordance with DIN EN 1822-3 and ISO 29463-3
- Simple use of different test aerosols, such as NaCl / KCl or DEHS (others on request)
- Easily movable dilution cascades with factors of 10, 100, 1,000 and 10,000 for measurements with salt or DEHS
- Simple measurement of the fraction separation efficiency and determination of the MPPS range
- High reproducibility of the testing method
- Flexible filter test software FTControl
- Easy to operate, even untrained personnel can be instructed quickly in the use of the equipment
- Cleaning can be performed autonomously by the customer
- Short set-up times, fast throughput times
- Mobile setup, easy to move on castors
- Validation of the clear function of individual components and the overall system during pre-delivery acceptance testing and upon delivery
- Reliable operation
- Low-maintenance
- The unit will reduce your operating costs

Datasheet

<i>Parameter</i>	<i>Description</i>
Measurement range (size)	U-SMPS 2050: 10 – 800 nm
Volume flow	0.54 – 16 m ³ /h (pressurized operation)
Power supply	115/230 V, 50/60 Hz
Dimensions	approx. 600 • 1,800 • 900 mm (W • H • D)
Inflow velocity	1.5 – 40 cm/s (others on request)
Differential pressure measurement	0 – 2,500 Pa (others on request)
Test area of the medium	100 cm ²
Aerosols	Dusts (e. g. SAE dusts), salts (e. g. NaCl, KCl), liquid aerosols (e. g. DEHS)
Compressed air supply	6 – 8 bar

Applications

- For filter media and small filter elements
- product development/ production control
- Test possibilities with regard to EN 1882-3 (HEPA/ULPA) and ISO 29463-3
- Fractional efficiency measurement in the range from approx. 20 nm up to 1 µm

Palas GmbH
Partikel- und Lasermesstechnik
Greschbachstrasse 3 b
76229 Karlsruhe
Germany

Managing Partner:
Dr.-Ing. Maximilian Weiß
Commercial Register:
register court: Mannheim
company registration number: HRB 103813
USt-Id: DE143585902



Contact: E-Mail: mail@palas.de Internet: www.palas.de Tel: +49 (0)721 96213-0 Fax: +49 (0)721 96213-33